

**Oracle Utilities Customer Care and Billing
Release 2.5.0**

Utility Reference Model

4.2.1.1a Read Meter

August 2016

Oracle Utilities Customer Care and Billing Release 2.5.0 Utility Reference Model 4.2.1.1a Read Meter

Copyright © 2016, Oracle and/or its affiliates. All rights reserved.

This software and related documentation are provided under a license agreement containing restrictions on use and disclosure and are protected by intellectual property laws. Except as expressly permitted in your license agreement or allowed by law, you may not use, copy, reproduce, translate, broadcast, modify, license, transmit, distribute, exhibit, perform, publish, or display any part, in any form, or by any means. Reverse engineering, disassembly, or decompilation of this software, unless required by law for interoperability, is prohibited.

The information contained herein is subject to change without notice and is not warranted to be error-free. If you find any errors, please report them to us in writing.

If this is software or related documentation that is delivered to the U.S. Government or anyone licensing it on behalf of the U.S. Government, then the following notice is applicable:

U.S. GOVERNMENT END USERS: Oracle programs, including any operating system, integrated software, any programs installed on the hardware, and/or documentation, delivered to U.S. Government end users are "commercial computer software" pursuant to the applicable Federal Acquisition Regulation and agency-specific supplemental regulations. As such, use, duplication, disclosure, modification, and adaptation of the programs, including any operating system, integrated software, any programs installed on the hardware, and/or documentation, shall be subject to license terms and license restrictions applicable to the programs. No other rights are granted to the U.S. Government.

This software or hardware is developed for general use in a variety of information management applications. It is not developed or intended for use in any inherently dangerous applications, including applications that may create a risk of personal injury. If you use this software or hardware in dangerous applications, then you shall be responsible to take all appropriate fail-safe, backup, redundancy, and other measures to ensure its safe use. Oracle Corporation and its affiliates disclaim any liability for any damages caused by use of this software or hardware in dangerous applications.

Oracle and Java are registered trademarks of Oracle and/or its affiliates. Other names may be trademarks of their respective owners.

Intel and Intel Xeon are trademarks or registered trademarks of Intel Corporation. All SPARC trademarks are used under license and are trademarks or registered trademarks of SPARC International, Inc. AMD, Opteron, the AMD logo, and the AMD Opteron logo are trademarks or registered trademarks of Advanced Micro Devices. UNIX is a registered trademark of The Open Group.

This software or hardware and documentation may provide access to or information about content, products, and services from third parties. Oracle Corporation and its affiliates are not responsible for and expressly disclaim all warranties of any kind with respect to third-party content, products, and services unless otherwise set forth in an applicable agreement between you and Oracle. Oracle Corporation and its affiliates will not be responsible for any loss, costs, or damages incurred due to your access to or use of third-party content, products, or services, except as set forth in an applicable agreement between you and Oracle.

Contents

4.2.1.1a Read Meter

4.2.1.1a Read Meter	1
Brief Description	2
Actors/Roles	2
Business Process Diagrams	3
Read Meter Process Model - Page 1	3
Read Meter Process Model - Page 2	4
Read Meter Detailed Process Model Description	5
1.0 Search for Meter	6
1.1 5.1.5.1 CC&B v2.5 Manage Meter Site	6
1.2 Evaluate Meter Information	6
1.3 Evaluate Meter Read	6
1.4 Enter Meter Read	6
1.5 Enter Office Estimated Meter Read	7
1.6 Request Add Field Activity	7
1.7 Add Field Activity	7
1.8 Enter Changes	7
1.9 Update Read	7
2.0 Select Meters Required to Be Read on Business Date	8
2.1 Retrieve Read Schedule, Route, Pending Meter Read Information	8
2.2 Create Flat File for Download	8
2.3 Receive Flat File	9
2.4 Accept Downloaded Information in Reading Software/Handheld Devices	9
2.5 Obtain Read	9
2.6 Enter Reason for Missed Read as Remark in Reading Software	9
2.7 Create Flat File of Reads for Upload	10
2.8 Send Flat File	10
Meter Read Types	11
Related Training	12

4.2.1.1a Read Meter

This section provides a description of the “Read Meter” business process, including:

- ◆ [Brief Description](#)
 - ◆ [Actors/Roles](#)
- ◆ [Business Process Diagrams](#)
 - ◆ [Read Meter Process Model - Page 1](#)
 - ◆ [Read Meter Process Model - Page 2](#)
- ◆ [Read Meter Detailed Process Model Description](#)
- ◆ [Meter Read Types](#)
- ◆ [Related Training](#)

Brief Description

Business Process: 4.2.1.1a CC&B v2.5 Read Meter

Process Type: Sub-Process

Parent Process: 4.2.1 CC&B v2.5 Collect and Process Meter Read and Miscellaneous Charges

Sibling Processes:

- 4.2.2 CC&B v2.5 Manage Bill
- 5.3.2.1 CC&B v2.5 Manage Field Activities and Field Orders
- 4.2.1.2aCC&B v2.5 Load Meter Reads
- 4.2.1.3aCC&B v2.5 Validate Meter Reads
- 4.2.1.4 CC&B v2.5 Manage Consumption Data Reporting

This process describes the cyclical meter reading process for meter service points as well as how to add and change ad hoc meter reads. Most organizations read their meters in assign routes with specific schedules. In addition, there are times when re-reads are required for verification, are obtained as part of another task, submitted by the Customer, or entered by a CSR or Authorized User.


Actors/Roles

The Read Meter business process involves the following actors and roles:

- **CSR:** CSR or Authorized User of the Customer Care and Billing application.
- **CC&B:** The Customer Care and Billing application. Steps performed by this actor/role are performed automatically by the application, without the need for user initiation or intervention.
- **A/P A/R Software:** Accounts Payable or Accounts Receivable Software (General Ledger)
- **Meter Reader/Technician:** A technician is routed to the field to collect reads.


Business Process Diagrams

Read Meter Process Model - Page 1

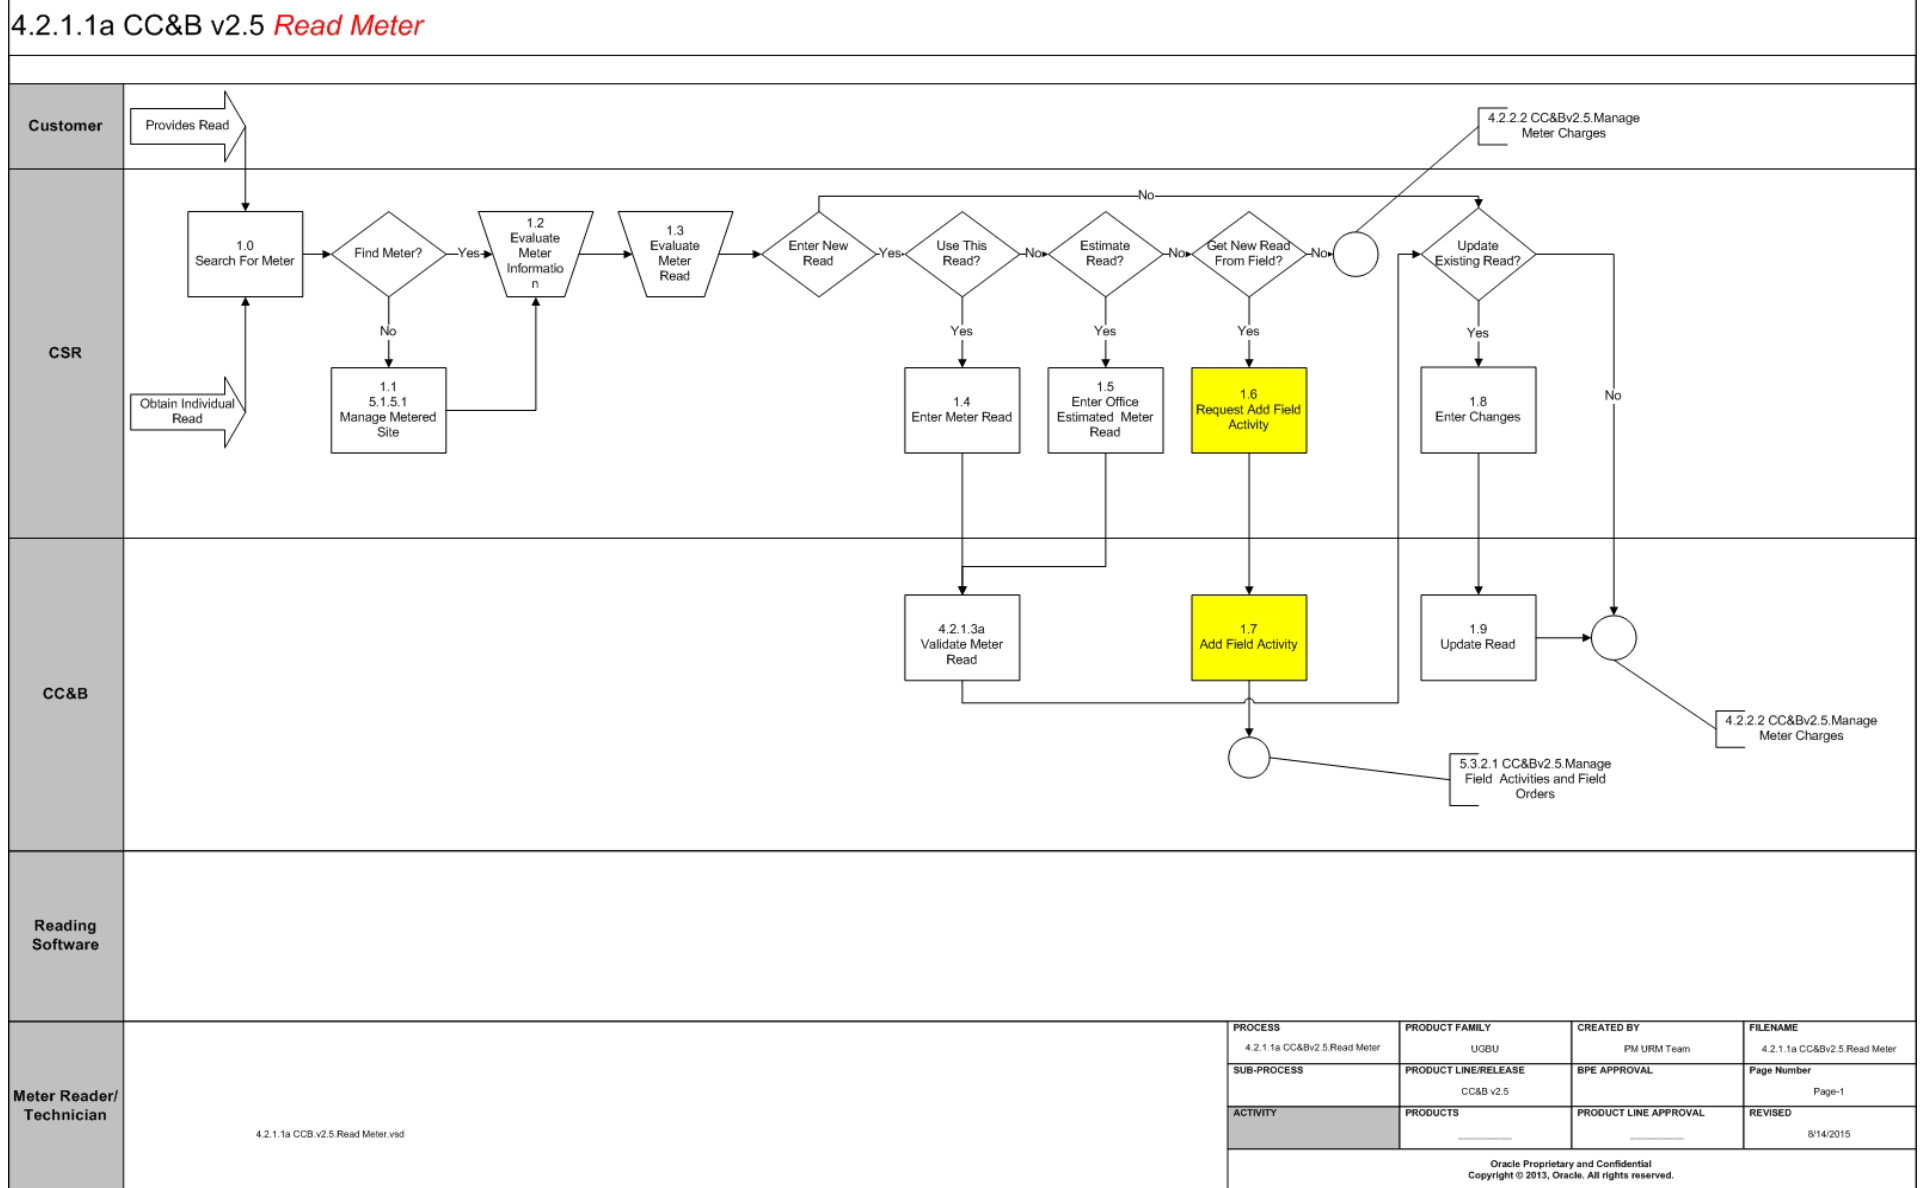

Read Meter Process Model - Page 2

4.2.1.1a. CC&B v2.5 *Read Meter*

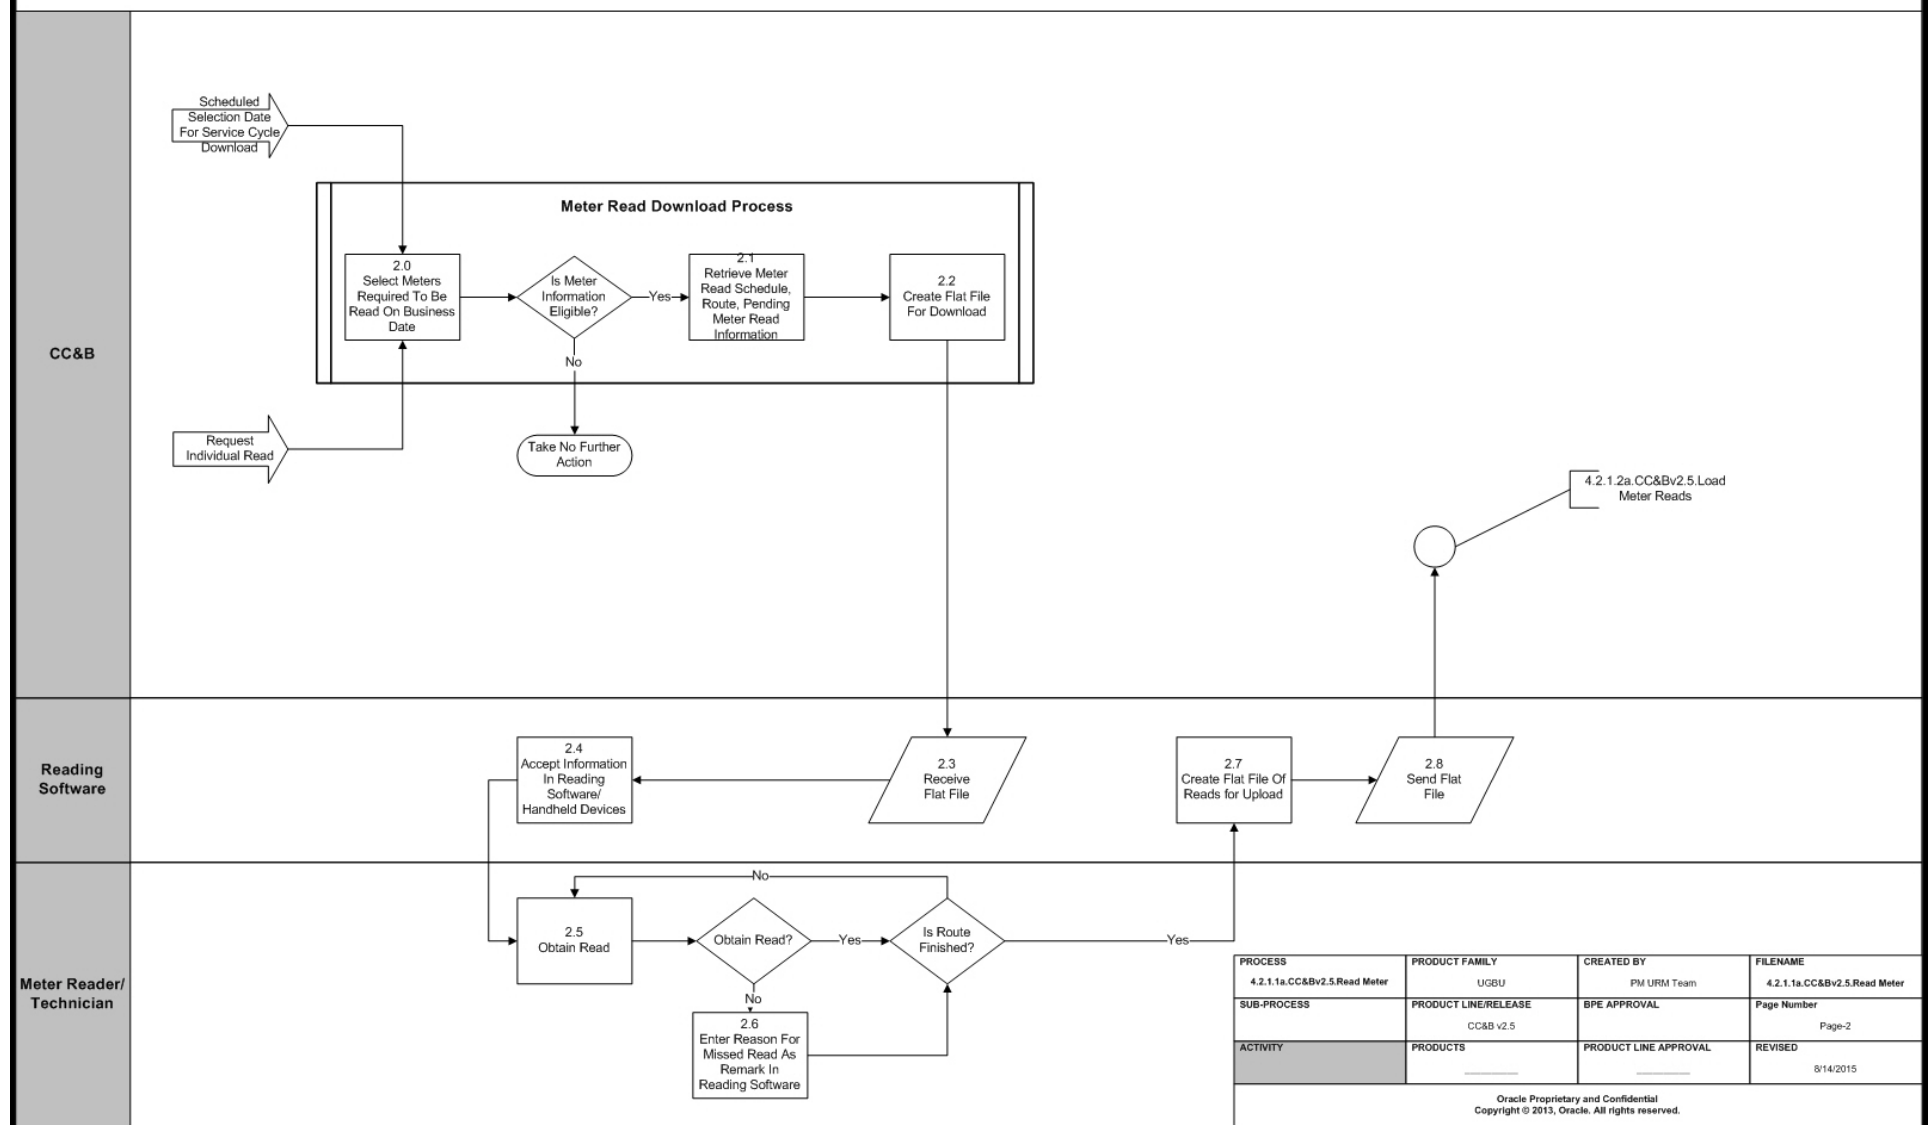

Read Meter Detailed Process Model Description

This section provides a detailed description of the “Read Meter” business process, including:

- ♦ 1.0 Search for Meter
- ♦ 1.1 5.1.5.1 CC&B v2.5 Manage Meter Site
- ♦ 1.2 Evaluate Meter Information
- ♦ 1.3 Evaluate Meter Read
- ♦ 1.4 Enter Meter Read
- ♦ 1.5 Enter Office Estimated Meter Read
- ♦ 1.6 Request Add Field Activity
- ♦ 1.7 Add Field Activity
- ♦ 1.8 Enter Changes
- ♦ 1.9 Update Read
- ♦ 2.0 Select Meters Required to Be Read on Business Date
- ♦ 2.1 Retrieve Read Schedule, Route, Pending Meter Read Information
- ♦ 2.2 Create Flat File for Download
- ♦ 2.3 Receive Flat File
- ♦ 2.4 Accept Downloaded Information in Reading Software/Handheld Devices
- ♦ 2.5 Obtain Read
- ♦ 2.6 Enter Reason for Missed Read as Remark in Reading Software
- ♦ 2.7 Create Flat File of Reads for Upload
- ♦ 2.8 Send Flat File

1.0 Search for Meter

Reference: [Read Meter Process Model - Page 1 on page 3](#) for the associated business process diagram.

Actor/Role: CSR

Description: The CSR or Authorized User searches for the Meter to enter a read. The read typically is provided by the Customer, exception processing, or a missed read during the meter read process. The Meter number or Badge Number as referenced in CC&B may be used to search for the Meter. Alternate search methods are used with the Meter/Item Search Notebook.

1.1 5.1.5.1 CC&B v2.5 Manage Meter Site

Reference: [Read Meter Process Model - Page 1 on page 3](#) for the associated business process diagram.

Actor/Role: CSR

Description: If the Meter cannot be located in CC&B, the CSR or Authorized User, may add the meter to inventory in CC&B. Refer to 5.1.5.1 CC&B v2.5 Manage Meter Site.

Entities to Configure

- Meter Type
- Meter Configuration Type
- Meter Model and Manufacturer

1.2 Evaluate Meter Information

Reference: [Read Meter Process Model - Page 1 on page 3](#) for the associated business process diagram.

Actor/Role: CSR

Description: The CSR or Authorized User reviews and validates meter type information including what consumption the meter measures, number of dials, meter constant or meter multiplier, and how the meter is used to calculate consumption.

1.3 Evaluate Meter Read

Reference: [Read Meter Process Model - Page 1 on page 3](#) for the associated business process diagram.

Actor/Role: CSR

Description: The CSR or Authorized User compares the read to be entered against read history for this meter as well as consumption trends for the service point. The CSR or Authorized User verifies whether or not other reads are already entered for the same time period and makes comparisons.

1.4 Enter Meter Read

Reference: [Read Meter Process Model - Page 1 on page 3](#) for the associated business process diagram.

Actor/Role: CSR

Description: The CSR or Authorized User accepts the read and enters the meter read information.

1.5 Enter Office Estimated Meter Read

Reference: [Read Meter Process Model - Page 1 on page 3](#) for the associated business process diagram.

Actor/Role: CSR

Description: The CSR or Authorized User enters the office-estimated meter read information.

1.6 Request Add Field Activity

Reference: [Read Meter Process Model - Page 1 on page 3](#) for the associated business process diagram.

Actor/Role: CSR

Description: It is determined a new read is required from the field. The CSR or Authorized User enters required information to obtain a new read. Refer to 4.2.2 CC&B v2.5 Manage Bill.

Entities to Configure

- Field Activity Type
- Field Activity Profile
- Field Service Controls

1.7 Add Field Activity

Reference: [Read Meter Process Model - Page 1 on page 3](#) for the associated business process diagram.

Actor/Role: CC&B

Description: The field activity is added in CC&B. Refer to 5.3.2.1 CC&B v2.5 Manage Field Activities and Field Orders.

1.8 Enter Changes

Reference: [Read Meter Process Model - Page 1 on page 3](#) for the associated business process diagram.

Actor/Role: CSR

Description: The CSR or Authorized user examines an existing read to determine if updates are required. Based on business rules, typically the only field the CSR or Authorized User modifies is the Use on Bill flag field. It is recommended to maintain an audit trail of all reads entered. The best practices approach is to remove the use on bill flag on a particular read if it is incorrect or will not be used for billing. The CSR or Authorized User can enter a new read as needed.

1.9 Update Read

Reference: [Read Meter Process Model - Page 1 on page 3](#) for the associated business process diagram.

Actor/Role: CC&B

Description: CC&B is updated with changes for the read. Refer to 4.2.2 CC&B v2.5 Manage Bill.

Entities to Configure

- Meter Read Type
- Meter Read Remark
- Characteristics related to Meter Read
- Meter Read source
- Meter Read Instructions (Related to Premise)

- Meter Read warnings (Related to Premise)

Available Algorithms

- CI_MREAD_BO - Determine Meter Read BO. This algorithm is defined on the MO and allows a business object to be used.
- CI_MeterReadAudit Meter Read Audit for Auditing Purpose only when Auditing is on.

Business Objects

- CI_MeterReadAudit Meter Read Audit for Auditing Purpose only when Auditing is on

2.0 Select Meters Required to Be Read on Business Date

Reference: [Read Meter Process Model - Page 1 on page 3](#) for the associated business process diagram.

Actor/Role: CC&B

Description: The scheduled selection date is reached. This is the date read information is available to Field Operations staff for reading. Requests for off cycle reads are received and available to Field Operations staff.

2.1 Retrieve Read Schedule, Route, Pending Meter Read Information

Reference: [Read Meter Process Model - Page 1 on page 3](#) for the associated business process diagram.

Actor/Role: CC&B

Description: This process looks for all meter read cycle schedules with a scheduled selection date on or before the given business date with routes not yet generated. For each record found this process creates a Meter Read schedule route record for every route in the cycle. This process reviews all the Meter Read schedule route records flagged for download and creates a record for every meter in a given route flagged as available for download. The system also selects the service points in the meter read cycle for download. Refer to 4.2.1.5 Maintain Meter Read Schedule.

Entities to Configure

- Service Schedule
- Service Cycle

Process Names

- MSR - Create MR Schedule Routes. This process looks for all meter read cycle schedules with routes not generated. Route Records are created for every route in cycle
- MDS - Create Download Staging. This process creates download staging records for meters linked to every service point in route

2.2 Create Flat File for Download

Reference: [Read Meter Process Model - Page 1 on page 3](#) for the associated business process diagram.

Actor/Role: CC&B

Description: This process reads all records marked for download with a given Batch Control ID and run number, and creates the flat file for Field Operations' various meter read software applications.

Process Names

- MDL - Create Download Flat File

2.3 Receive Flat File

Reference: [Read Meter Process Model - Page 1 on page 3](#) for the associated business process diagram.

Actor/Role: Reading Software

Description: The reading software in Field Operations receives the flat file.

2.4 Accept Downloaded Information in Reading Software/Handheld Devices

Reference: [Read Meter Process Model - Page 1 on page 3](#) for the associated business process diagram.

Actor/Role: Reading Software

Description: Meter Read Information is downloaded to reading software and/or handheld devices in preparation for reading in the field.

2.5 Obtain Read

Reference: [Read Meter Process Model - Page 1 on page 3](#) for the associated business process diagram.

Actor/Role: Meter Reader/Technician

Description: A technician is routed to the field to collect reads.

2.6 Enter Reason for Missed Read as Remark in Reading Software

Reference: [Read Meter Process Model - Page 1 on page 3](#) for the associated business process diagram.

Actor/Role: Meter Reader/Technician

Description: At times it may not be possible to obtain the read from the customer's meter. An obstruction, clouded glass, or animal may prevent the reader the reader from getting the read. An entry is made in the reading software to communicate the reason the read was not obtained. Comments from the Meter Reader can trigger a Field Activity, Customer Contact or Bill Message. Refer to 4.2.1.2a Load Meter Reads

Entities to Configure

- Field Activity Type
- Bill Message
- Customer Contact Class and Contact Type
- MR Remarks

Available Algorithms

- CI_MRRCREAM - This algorithm creates an Account Message to be placed on bill (Create “contact CSR” account message).
- CI_MRRCRECC - This algorithm creates a Create Service Customer Contact.
- CI_CREMRCSE - This algorithm creates a case from Meter Read Remark.
- MRR-SIO - This algorithm creates M-SIO Meter - service investigation Field Activity.
- CI_CRESIOFA - Create “SIO” field activity
- C1-MeterRead - Determine Meter Read BO
- WX-CustomerMeterRead - Initiated by Self Service

Process Names

- CI_MREAD_BO - Determine Meter Read BO
- MRRA - Background process read remark activation

2.7 Create Flat File of Reads for Upload

Reference: [Read Meter Process Model - Page 1 on page 3](#) for the associated business process diagram.

Actor/Role: Reading Software

Description: The reading software prepares a flat file containing reads and meter information for Upload to CC&B.

2.8 Send Flat File

Reference: [Read Meter Process Model - Page 1 on page 3](#) for the associated business process diagram.

Actor/Role: Reading Software

Description: Reading Software in Field Operations sends a flat file to CC&B for Upload to CC&B.

Meter Read Types

The following meter read types are available:

Read Type	Description
Billing Force	Meter reads with this value are entered by a billing administrator who wants to force billing to bill a customer for a given amount of consumption.
Verified	A meter reader using a handheld device records meter reads with this value. The handheld device deems a read as “verified” if the meter reader typed the same dial reading in twice. Some organizations have their handhelds programmed to require the double entry of dial readings when the entered value is outside normative values (i.e., the resultant consumption fails high / low checks).
Regular	A meter reader using a handheld device records meter reads with this value. See the description for “verified” above for the difference between a “regular” and a “verified” reading.
Customer Read	A customer provides meter reads with this value.
System Prorate	Meter reads with this value are created by the system automatically when prorating normal cycle-based reads for use with an off-cycle start service or stop service.
Office Estimate	Meter reads with this value are informed guesses of consumption. These would be used when there was no real reading (i.e., a regular or verified reading), and the system was not allowed to estimate consumption (for whatever reason). This value is rarely used.
Service Provider Estimate	Meter reads with this value are estimates of consumption made by a 3rd party service provider, such as an MDMA, the distribution company, or an energy supply company.
System Estimate	The billing process creates meter reads with this value when a reading cannot be found and the service agreement allows estimation.
No Read	Meter reads with this value are entered to indicate that a read was purposefully not performed (for whatever reason - mad dog, nasty rose bush, deep snow, etc.). A read with this value is not a read at all; it's just an audit trail.

Related Training

The following User Productivity Kit (UPK) modules provide training related to this business process:

- Oracle Utilities UPK for Customer Care and Billing, Administrative Setup
- Oracle Utilities UPK for Customer Care and Billing, Rating and Billing
- Oracle Utilities UPK for Customer Care and Billing, Rating and Billing for Interval Data
- Oracle Utilities UPK for Customer Care and Billing, User Tasks
- Oracle Utilities UPK for Customer Care and Billing, Credit and Collections